

**Analysis of Residual Solvents in Pharmaceuticals
by Water-Soluble Samples Using N₂ Carrier
(JP18, USP 467)**

The Japanese Pharmacopoeia 18th Edition (JP18) and the United States Pharmacopoeia (USP) General Chapter <467> Residual Solvents provide test methods for residual solvents in pharmaceuticals mainly using headspace gas chromatography (GC). Residual solvents in pharmaceuticals are classified from Class 1 to 3 based on their potential human health risk. Since these compounds are strictly controlled, highly sensitive analysis is required. Helium (He) is generally used as the carrier gas, but as He supply shortages have become an issue recently, analysis using an alternative carrier gas such as N₂ has also been in demand lately. Any method changes, such as substituting He with an alternate carrier gas, must be validated according to USP General Chapter <1467> Residual Solvents—Verification of Compendial Procedures and Validation of Alternative Procedures.

This article introduces a JP18-compliant analysis of water-soluble samples for Class 1 and 2 residual solvents using N₂ as the carrier gas.

N. Iwasa, T. Wada

**Instrument Configuration and
Analysis Conditions**

Class 1 and 2 standard solutions were prepared and measured in accordance with Procedure A and B of JP18, using Shimadzu HS-20 headspace gas sampler connected to Nexis™ GC-2030 gas chromatograph. The two procedures differ in the type of column, the column temperature and the split ratio. Table 1 lists the GC and HS-20 analysis conditions used in this experiment.

Table 1 **Water-Soluble Sample Analysis Conditions**

GC analysis conditions (Procedure A and B)	
Model	: Nexis™ GC-2030
Detector	: FID-2030 flame ionization detector
Column	: A) SH-Rxi™-624 Sil MS (0.32 mm I.D. × 30 m, d.f.= 1.8 μm) B) SH-Stabilwax™ (0.32 mm I.D. × 30 m, d.f.= 0.25 μm)
Column temp.	: A) 40 °C (20 min) - 10 °C/min - 240 °C (20 min) Total 60 mins B) 50 °C (20 min) - 6 °C/min - 165 °C (20 min) Total 59.17 mins
Injection mode	: A) Split 1:5 B) Split 1:10
Carrier gas controller	: Linear velocity (N ₂)
Linear velocity	: 35 cm/sec
Detector temp.	: 250 °C
FID H ₂ flow rate	: 32 mL/min
FID make up flow rate	: 24 mL/min (N ₂)
FID air flow rate	: 200 mL/min
Injection volume	: 1 mL
HS-20 analysis conditions (same for Procedure A and B)	
Oven temp.	: 80 °C
Sample line temp.	: 110 °C
Transfer line temp.	: 120 °C
Vial shaking level	: Off
Vial volume	: 20 mL
Vial equilibrating time	: 60 min
Vial pressurizing time	: 1 min
Vial pressure	: 75 kPa
Loading time	: 0.5 min
Needle flush time	: 5 min

**Analysis of Class 1 Standard Solution
(Water-Soluble Sample)**

The analysis results for Procedure A and B are shown in Fig. 1 and 2 respectively. Table 2 and 3 summarize the S/N ratios and the repeatability of Procedure A and B respectively.

The results obtained with Procedure A satisfied the requirements of JP18 which states that “the S/N ratio for 1,1,1-trichloroethane in the Class 1 standard solution is not less than 5 and the relative standard deviation of each peak area is not more than 15 %.” Satisfactory results were also obtained with Procedure B, as “the S/N ratio for benzene in the Class 1 standard solution is not less than 5 and the relative standard deviation of each peak area is not more than 15 %.”

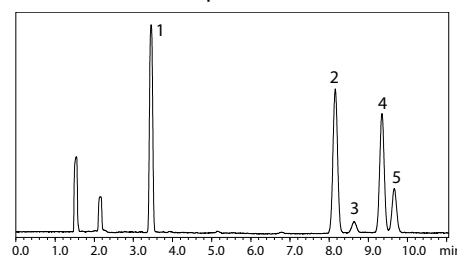


Fig. 1 **Chromatogram of Class 1 Standard Solution by Procedure A (Water-Soluble Sample)**

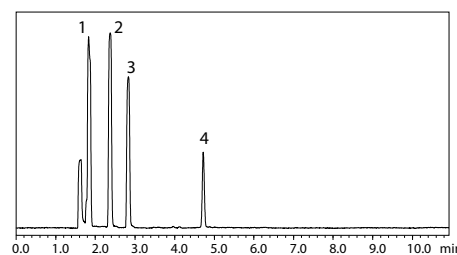


Fig. 2 **Chromatogram of Class 1 Standard Solution by Procedure B (Water-Soluble Sample)**

Table 2 **S/N Ratio and Repeatability of Class 1 Standard Solution (Procedure A)**

Peak No.	Compound	S/N ratio ^{*1}	%RSD (n=6) ^{*1}
1	1,1-Dichloroethane	263	1.81
2	1,1,1-Trichloroethane	242	1.74
3	Carbon tetrachloride	18	2.72
4	Benzene	204	2.08
5	1,2-Dichloroethane	69	1.56

Table 3 **S/N Ratio and Repeatability of Class 1 Standard Solution (Procedure B)**

Peak No.	Compound	S/N ratio ^{*1}	%RSD (n=6) ^{*1}
1	1,1-Dichloroethane	174	1.77
2	1,1,1-Trichloroethane	181	2.18
3	+Carbon tetrachloride Benzene	142	1.12
4	1,2-Dichloroethane	105	1.02

In Table 2 and 3, the items specified in JP18 are shown in red.

*1 The S/N ratios and relative standard deviation (%RSD) are reference values and not intended to be guaranteed values.

■ Analysis of Class 2 Standard Solution (Water-Soluble Sample)

Fig. 3 and 4 below show the analysis results for Procedure A and B (Black: Class 2 mixture A standard solution (Class 2A), Pink: Class 2 mixture B standard solution (Class 2B), Blue: MIBK).

For system suitability, JP18 specifies that “the resolution between acetonitrile and methylene chloride in the Class 2 mixture A standard solution is not less than 1.0” when using Procedure A, and “the resolution between acetonitrile and cis-1,2-dichloroethene in the Class 2 mixture A standard solution is not less than 1.0” when using Procedure B. Satisfactory results were obtained with both procedures.

* The resolutions shown in the Fig. 3 and 4 are reference values and not guaranteed.

■ Conclusion

Using a N₂ carrier gas, the analysis achieved the accuracy levels required by Japanese Pharmacopoeia 18th Edition and USP General Chapters <467> and <1467>. In the analysis of residual solvents in water-soluble pharmaceuticals using the headspace GC method, satisfactory results comparable to those with He carrier gas were obtained with N₂ as the carrier gas.

For information about using a H₂ carrier for analysis of residual solvents in pharmaceuticals using water-soluble samples, refer to Application News 01-00176-EN.

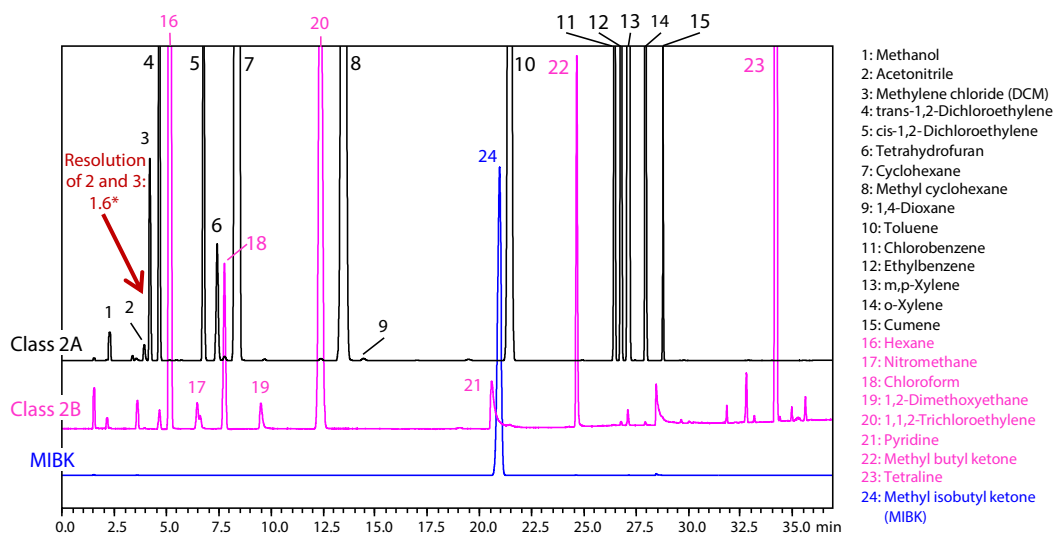


Fig. 3 Chromatogram of Class 2 Standard Solution by Procedure A (Water-Soluble Sample)

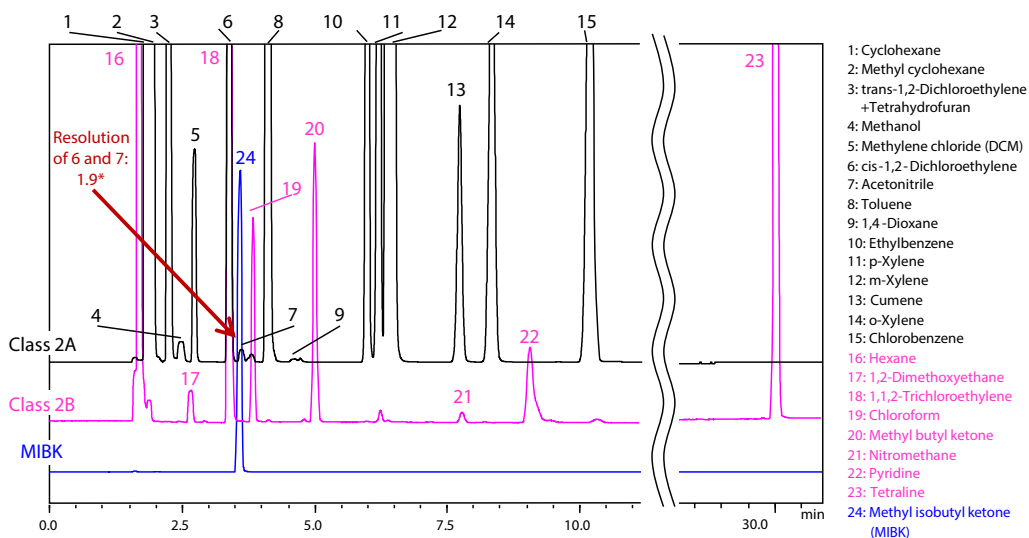


Fig. 4 Chromatogram of Class 2 Standard Solution by Procedure B (Water-Soluble Sample)

Nexis is a trademark of Shimadzu Corporation in Japan and/or other countries.

Rxi and Stabilwax are either trademarks or registered trademarks of Restek Corporation in the United States and/or other countries.



Shimadzu Corporation

www.shimadzu.com/an/

For Research Use Only. Not for use in diagnostic procedure.

This publication may contain references to products that are not available in your country. Please contact us to check the availability of these products in your country.

The content of this publication shall not be reproduced, altered or sold for any commercial purpose without the written approval of Shimadzu. Shimadzu disclaims any proprietary interest in trademarks and trade names used in this publication other than its own. See <http://www.shimadzu.com/about/trademarks/index.html> for details.

The information contained herein is provided to you "as is" without warranty of any kind including without limitation warranties as to its accuracy or completeness. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication. This publication is based upon the information available to Shimadzu on or before the date of publication, and subject to change without notice.

First Edition: Jun. 2020
Second Edition: Jul. 2021