

# Application News

## No. i271

### Material Testing Machine

## Measurement of Paint Bake Hardening of Metals Conforming to JIS G 3135 Annex A

### Introduction

Automobiles have become an indispensable part of our daily lives, but in recent years, application of various materials such as carbon fiber reinforced plastic and high tensile strength steel has been studied with the aim of reducing auto body weight in order to improve fuel economy and reduce CO<sub>2</sub> emissions, and many such materials have been applied practically.

However, the required material properties differ in each automotive component. In particular, materials with high dent resistance, i.e., resistance to depressions caused by impact by small stones or other objects that bounce up during travel, is demanded in doors, hoods, and other outer panels. Increasing the contents of carbon and nitrogen to increase yield strength are effective for improving dent resistance, but press forming becomes difficult, and the forming defect called "surface deflection" increases. On the other hand, in order to improve formability and secure high surface accuracy, soft materials with low yield strength are required.

Bake-hardening steel sheets (BH steel sheets) are used to satisfy the mutually-contradictory requirements of high formability and high dent resistance. BH steel sheets are a type of steel sheet that is soft and has high formability at the time of forming, and then hardens when dried with heat (baked) in the subsequent painting process.

This article introduces an example in which tests were conducted in accordance with JIS G 3135 Annex A in order to obtain the paint bake-hardening amount (BH amount) of SPCC, SPFC590, and SPFC1180 steels.

Y. Kamei

### Paint Bake-Hardening Amount Calculation Method

Fig. 1 shows the image of measurement of the BH amount as provided in JIS G 3135 Annex A, together with the terminology. The BH amount ( $\sigma_{BH}$ ) is evaluated by the amount of rise in yield stress when heat treatment corresponding to the baking finish process is performed with a steel material to which prestrain has been applied. The measurement procedure is shown below.

- (1) Perform a tensile test at a speed of 10 to 30 MPa/s, obtain the prestrain (work hardening) stress  $R_{WH}$  when the total elongation of the specimen reaches 2 %, and then release the force.
- (2) Conduct heat treatment of the specimen in (1) at 170 °C for 20 min, then air cooling.
- (3) Obtain the strain aging yield stress  $R_{SA}$  by conducting a tensile test of the specimen which was heat-treated according to (2).  $\sigma_{BH} = R_{SA} - R_{WH}$ .

In this test, processing to calculate the numerical values obtained by two tensile tests is necessary. With the conventional method,  $\sigma_{BH}$  could not be calculated using software alone. However, Shimadzu TRAPEZIUMX-V materials testing software enables calculation of the value of  $\sigma_{BH}$  by reading past test results. In this experiment, the test results when prestrain stress was measured were read from the test results of the strain aging yield stress measurement, and  $\sigma_{BH}$  was calculated in the software.

### Test Conditions

Table 1 and Table 2 show the test conditions and specimen information respectively. For comparison, three tests were carried out with each of three types of steel, SPCC, SPFC590, and SPFC1180, and the average values were obtained. Fig. 2 shows the condition of JIS Test. In these measurements, the tests were carried out using Shimadzu hydraulic flat grips, which feature strong gripping force, in order to conduct the test of the high strength SPFC material without slipping in the grips.

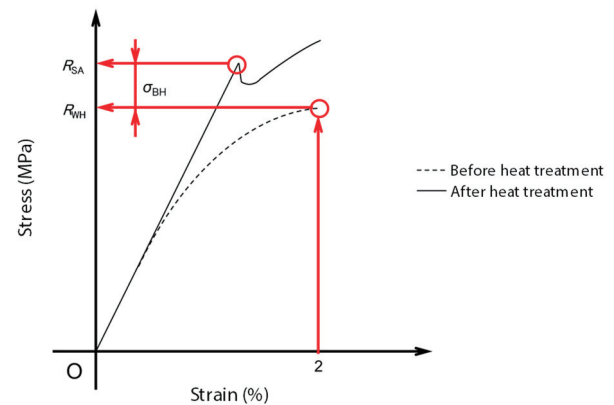


Fig. 1 Image of Measurement by JIS G 3135

Table 1 Test Conditions

Instrument	: AGX™-100kNV
Load cell	: 100 kN
Test jig	: 100 kN hydraulic flat grip
Grip face	: Single-side file-teeth grip face for flat grip
Extensometer	: SSG50-10H
Software	: TRAPEZIUMX-V single
Test speed	: 10 MPa/s (load until extensometer output of 2 %)
Heat treatment conditions	: Heating at 170 °C for 20 min, followed by air cooling

Table 2 Specimen Information

Specimen types	: SPCC, SPFC590, SPFC1180
Number of specimens	: 3 specimens/type
Specimen geometry	: No. 5 dumbbell (JIS Z 2241)
Original dimensions of parallel portion	: Width 25 mm × thickness 1 mm

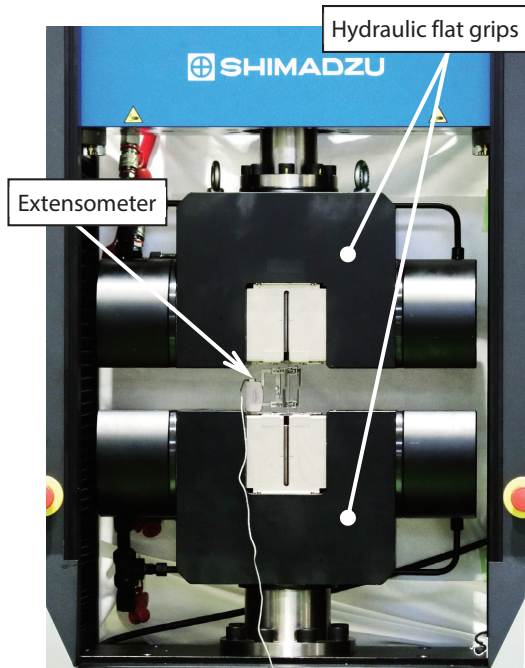


Fig. 2 Condition of JIS Test

### Test Results

Fig. 3, 4, and 5 show examples of the test results for SPCC, SPFC590, and SPFC1180, respectively. Strain on the horizontal axis is the value obtained by converting the output of the extensometer, and stress on the vertical axis is the value calculated based on the cross-sectional area of the parallel portion before applying prestrain. With all specimens, it can be understood that there are differences in the S-S curves before and after heat treatment. Table 3 shows the measured stress values and the calculated  $\sigma_{BH}$  for each type of specimen. The lowest  $\sigma_{BH}$  was obtained with SPFC590, and  $\sigma_{BH}$  increased in SPCC and SPFC1180 in that order.

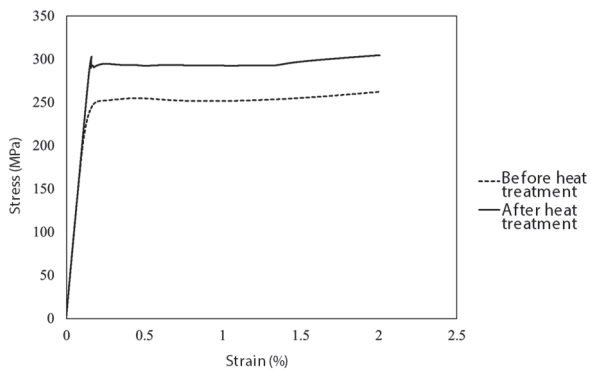


Fig. 3 Test Results of SPCC

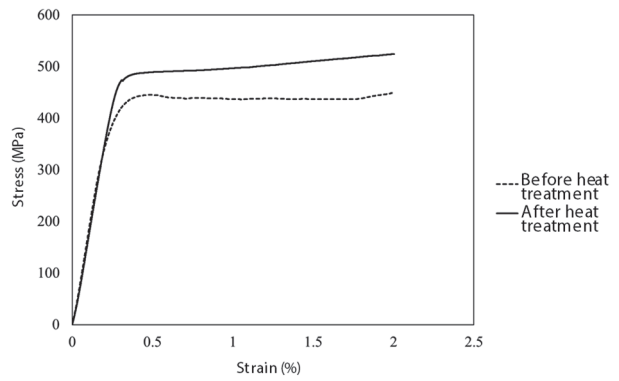


Fig. 4 Test Results of SPFC590

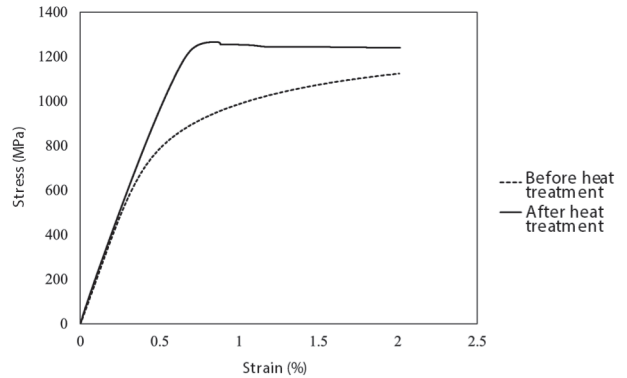


Fig. 5 Test Results of SPFC1180

Table 3 Summary of Test Results (Average of n=3)

	$R_{WH}$ (MPa)	$R_{SA}$ (MPa)	$\sigma_{BH}$ (MPa)
SPCC	261.0	297.7	36.7
SPFC590	447.4	472.5	25.1
SPFC1180	1119.3	1264.2	144.9

### Conclusion

This article introduced an example in which tests conforming to JIS G 3135 Annex A were conducted and  $\sigma_{BH}$  was calculated using Shimadzu TRAPEZIUMX-V materials testing software. In addition to tensile strength, percentage elongation after fracture, elastic modulus, and similar items provided in JIS Z 2241, the value of  $\sigma_{BH}$  becomes an important item in material selection of materials used in automotive outer panels such as doors and hoods.

Calculation of  $\sigma_{BH}$  conforming to JIS G 3135 Annex A is easily possible by using Shimadzu measurement system.

TRAPEZIUM and AGX are trademarks of Shimadzu Corporation in Japan and/or other countries.

First Edition: Sep. 2019



For Research Use Only. Not for use in diagnostic procedures.

This publication may contain references to products that are not available in your country. Please contact us to check the availability of these products in your country.

The content of this publication shall not be reproduced, altered or sold for any commercial purpose without the written approval of Shimadzu. Shimadzu disclaims any proprietary interest in trademarks and trade names used in this publication other than its own. See <http://www.shimadzu.com/about/trademarks/index.html> for details.

The information contained herein is provided to you "as is" without warranty of any kind including without limitation warranties as to its accuracy or completeness. Shimadzu does not assume any responsibility or liability for any damage, whether direct or indirect, relating to the use of this publication. This publication is based upon the information available to Shimadzu on or before the date of publication, and subject to change without notice.

Shimadzu Corporation

[www.shimadzu.com/an/](http://www.shimadzu.com/an/)